

Retractable Disposable Scalpel - Sterile

ABS Handle fitted with Stainless Steel Surgical Blade, individually packed

| Product | Product No | Unit | Product | Product No | Unit |
|---------------------------------|------------|-----------|---------------------------------|------------|-----------|
| 10 scalpels individually packed | | | 25 scalpels individually packed | | |
| 10 | 4901 | Box of 10 | 10 | 3901 | Box of 25 |
| 10A | 4902 | Box of 10 | 10A | 3902 | Box of 25 |
| 11P | 4991 | Box of 10 | 11P | 3991 | Box of 25 |
| 12 | 4904 | Box of 10 | 12 | 3904 | Box of 25 |
| 14 | 4919 | Box of 10 | 14 | 3919 | Box of 25 |
| 15 | 4905 | Box of 10 | 15 | 3905 | Box of 25 |
| 15C | 4921 | Box of 10 | 15C | 3921 | Box of 25 |
| 20 | 4906 | Box of 10 | 20 | 3906 | Box of 25 |
| 21 | 4907 | Box of 10 | 21 | 3907 | Box of 25 |
| 22 | 4908 | Box of 10 | 22 | 3908 | Box of 25 |
| 23 | 4910 | Box of 10 | 23 | 3910 | Box of 25 |
| 24 | 4911 | Box of 10 | 24 | 3911 | Box of 25 |
| 25A | 4915 | Box of 10 | 25A | 3915 | Box of 25 |
| Stitch Cutter | 4926 | Box of 10 | Stitch Cutter | 3926 | Box of 25 |
| | | | | | |
| 10R | 4990 | Box of 10 | 10R | 3990 | Box of 25 |

Retractable Disposable Scalpel - Non-Sterile

ABS Handle fitted with Stainless Steel Surgical Blade, bulk packed

| Product | Product No | Unit | Product | Product No | Unit |
|--------------------------|------------|------------|--------------------------|------------|------------|
| 500 scalpels bulk packed | | | 500 scalpels bulk packed | | |
| 10 | 4001 | Box of 500 | 21 | 4007 | Box of 500 |
| 10A | 4002 | Box of 500 | 22 | 4008 | Box of 500 |
| 11P | 4091 | Box of 500 | 23 | 4010 | Box of 500 |
| 12 | 4004 | Box of 500 | 24 | 4011 | Box of 500 |
| 14 | 4019 | Box of 500 | 25A | 4015 | Box of 500 |
| 15 | 4005 | Box of 500 | Stitch Cutter | 4026 | Box of 500 |
| 15C | 4021 | Box of 500 | | | |
| 20 | 4006 | Box of 500 | 10R | 4090 | Box of 500 |

Swann-Morton and the 'ring pattern' logo are registered trademarks of Swann-Morton Limited and related companies. The products shown are manufactured for use by trained health care professionals and can cause injury if used or handled incorrectly. The information and illustrations used in connection with the products shown on this leaflet are for general guidance only and users must seek proper training and instruction in their use before using or handling such products. Swann-Morton Limited exclude all liability for injury to the extent permitted by law.



Swann-Morton Ltd. Penn Works, Owlerton Green, Sheffield S6 2BJ Telephone: 0114 2344231, Sales 0114 234422 uksales@swann-morton.com, exportsales@swann-morton.com orders@swann-morton.com, www.swann-morton.com

RET4pp/issue 2 03/20

Finger on the Trigger

Scalpels by




Extend to Use and Retract for Safety






An extended Retractable Scalpel range with Sharps Safety compliance in mind.

The EU Council Directive 2010/32/EU accepted into UK law under the Health and Safety (Sharps Instruments in Healthcare) regulations 2013 aims to achieve the safest possible environment for Healthcare workers through the prevention of sharps related injuries. Medical devices incorporating engineered safety mechanisms and protection should be "considered" by staff as "part" of their risk assessment process alongside training and education in best practice when handling sharps. The Swann-Morton retractable safety scalpel is one such device and is now available in an extended range offering 15 blade shapes including a Safety Stitch Cutter.

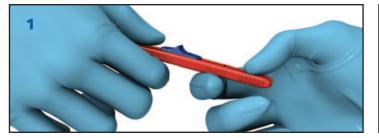


1 The high visibility red handle body contains a mid-safe passing notch into which the coloured slider is located whilst retracted so that the blade is held securely and safely when passing between members of the surgical team.

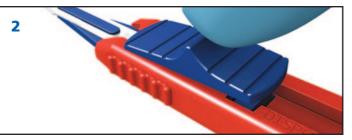

2 The user can expose the blade by placing downward pressure onto the sliding trigger and pushing it forward to engage the temporary usage position.



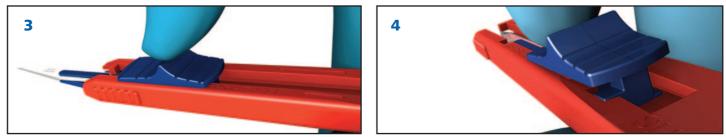

3 This forward lock is strengthened to prevent any uncontrolled retraction of the blade when coming into contact with hard surfaces or bone during use.







4 Once the procedure is finished and the count completed the trigger should be moved from the safe passing position towards the back of the handle body, where with a conscious amount of effort, it will engage the permanent locking position ready for final disposal in a sharps container.







Scan this code for more product information